



## COMMENT

### Tidal volume and helmet: Is the never ending story coming to an end?



A. Cortegiani<sup>a,\*</sup>, M. Ippolito<sup>a</sup>, M. Luján<sup>b</sup>, C. Gregoretti<sup>a</sup>

<sup>a</sup> Department of Surgical, Oncological and Oral Science (Di.Cir.On.S.), Section of Anesthesia, Analgesia, Intensive Care and Emergency, Policlinico Paolo Giaccone, University of Palermo, Via del vespro 129, 90127, Palermo, Italy

<sup>b</sup> Department of Pneumology Hospital de Sabadell, Universitat Autònoma de Barcelona, Parc Taulí, 1, 08208 Sabadell, Spain

Noninvasive ventilation (NIV) has been increasingly used in acute care setting with various indications<sup>1–3,4</sup> but its use in patients with acute hypoxic respiratory failure (AHRF) is controversial.<sup>5,6,7</sup>

Although spontaneous patient activity during mechanical ventilation (MV) may reduce the likelihood of ventilation-perfusion mismatch, especially in dependent regions, close to the diaphragm, high transmural vascular and transpulmonary pressure swing may worsen vascular leakage and increase tidal volume ( $V_t$ ), leading to self-inflicted lung injury (SILI).<sup>8</sup> From the clinical side, expiratory  $V_t$  of 6 mL/kg used in invasive MV during lung protective ventilation<sup>1</sup> is almost impossible to achieve in most of the patients receiving NIV for AHRF. This is particularly important in de novo AHRF patients undergoing NIV,<sup>1,2</sup> since large expiratory  $V_t$  may be generated<sup>9,10</sup> in assisted pressure controlled modes by the ventilator pressure and by the respiratory muscles.

**Abbreviations:** AHRF, acute hypoxic respiratory failure; CPAP, continuous positive airway pressure; ICU, intensive care unit; ILC, intentional leak single-limb vented circuit; IMV, invasive mechanical ventilation; MV, mechanical ventilation; NIV, noninvasive ventilation; SILI, self-inflicted lung injury; TDV, turbine driven NIV ventilator;  $V_t$ , tidal volume.

\* Corresponding author.

E-mail addresses: [andrea.cortegiani@unipa.it](mailto:andrea.cortegiani@unipa.it) (A. Cortegiani), [ippolito.mariachiara@gmail.com](mailto:ippolito.mariachiara@gmail.com) (M. Ippolito), [mlujan@tauli.cat](mailto:mlujan@tauli.cat) (M. Luján), [c.gregoretti@gmail.com](mailto:c.gregoretti@gmail.com) (C. Gregoretti).

In this setting, reliable monitoring of  $V_t$  and unintentional leaks is of the utmost importance. When using an intensive care unit (ICU) ventilator driven by high pressures in the double limb configuration, leaks are computed as the difference between inspired and expired  $V_t$ . As a consequence, the amount of  $V_t$  that the patient gets is usually quantified as expiratory  $V_t$ .

However, some points need to be clarified:

- 1) One characteristic of unintentional leaks is that they are dynamic, which means they can abruptly change during the inspiratory or expiratory phase of the respiratory cycle (even cycle by cycle). Therefore, expiratory  $V_t$  measurements using masks may cause concern, because measurements may become unreliable, unstable and difficult to continuously monitor {Carteaux:201dg}, where there may be unintentional expiratory leaks<sup>11</sup>;
- 2) Although there is a strong belief that preset  $V_t$  is equal to the real delivered  $V_t$ , in volume controlled mode using ICU ventilator driven by high pressures, one study found that  $V_t$  indicated by the ventilator was lower than the delivered  $V_t$ , with a difference that was often greater than 10% of the preset  $V_t$ .<sup>12</sup> This is also true during pressure controlled mode using NIV, where the direct measurement of flow (and its integration over the time, namely  $V_t$ ) by the pneumotachograph inside the ventilator, needs to be corrected for the compressible volume. This is the amount of gas which is compressed in the cir-

**Table 1** Differences in tidal volumes measured by turbine driven ventilator and lung simulator at different levels of PEEP in the bench study.

Simulated condition	(TDV-LS)PEEP 5 cmH <sub>2</sub> O	(TDV-LS) PEEP 8 cmH <sub>2</sub> O	(TDV-LS) PEEP 10cmH <sub>2</sub> O	(TDV-LS) PEEP 12 cmH <sub>2</sub> O	p Value
Restrictive	61 (3) <sup>o</sup> +§	104.4 (1.3)*+§	1.1 (1.6)*§	-11.9 (1.9)*+ <sup>o</sup>	<0.001

Data reported from Ref. 17. Data are expressed in ml and reported as mean ( $\pm$ SD). PEEP: positive end expiratory pressure; TDV: turbine driven ventilator; LS: lung simulator; (TDV-LS): difference between VT measurements by turbine driven ventilator and lung simulator.

\*Different from 5; <sup>o</sup>different from 8, +different from 10, §different from 12.


cuit and in the mask (the greater the internal volume of the mask the higher the compressible volume) for each cmH<sub>2</sub>O of pressure delivered by the ventilator during inspiration. Although most of ICU ventilators are usually equipped with algorithms to calculate and compensate for the compressible volume of the circuit,<sup>13</sup> they do not compensate for the mask internal volume or compliance;

Many companies manufacture dedicated turbine driven NIV ventilators (TDV) with a high pressure O<sub>2</sub> inlet to preset a given FiO<sub>2</sub> and an intentional leak single-limb vented circuit (ILC),<sup>11</sup> where V<sub>t</sub> is not measured but estimated.<sup>14</sup> Although this circuit configuration is extensively used, the accuracy of V<sub>t</sub> estimate depends on many factors, including the pressure decrease across the limb, especially where there are high unintentional leaks. This is the reason why some ventilators use a mathematical algorithm to calculate this pressure drop or they still measure pressure close to the mask. Finally, the V<sub>t</sub> and leakage estimation in the presence of random leaks remains a challenge when using ILC.<sup>1,14</sup> However, V<sub>t</sub> estimation has been found to have around 15% when compared to the real measured V<sub>t</sub> in restrictive disorders. This means that, when 500 ml of volume are generated, estimates may be around  $\pm$  75 ml, a bias not significantly different from the one measured by many pneumotachographs inside the ventilator.<sup>14</sup>

They may also allow better patient-ventilator synchrony than ICU pressure driven ventilators, even when coupled with their NIV algorithms.<sup>15</sup> Accuracy in estimating leakage is also crucial to improve patient-ventilator synchrony, especially when pneumatic (flow) trigger systems are used. Most of these systems automatically change their sensitivity level according to leakage estimates to avoid trigger asynchronies (autotriggering or ineffective efforts).

Another important concern during NIV in de novo AHRF is that, compared to IMV, it cannot often be used continuously on a daily basis. Although the use of total face mask may increase patient's tolerance and compliance to NIV and decrease unintentional leaks, the likelihood of maintaining patients under NIV with a mask round the clock for days is remote.

An alternative interface is the helmet, which consists of a transparent hood covering the patient's whole head with a soft collar neck seal.<sup>16</sup> It is kept in place by two armpit belts or by an annular extendable plastic ring positioned under an inflatable cushion that eliminates the need for armpits straps.<sup>16</sup> Helmet NIV resulted in higher levels of positive end expiratory pressure (PEEP) and a lower intubation rate in patients with AHRF in a single randomized controlled trial.<sup>16</sup> This study suggests that the helmet may allow more time on

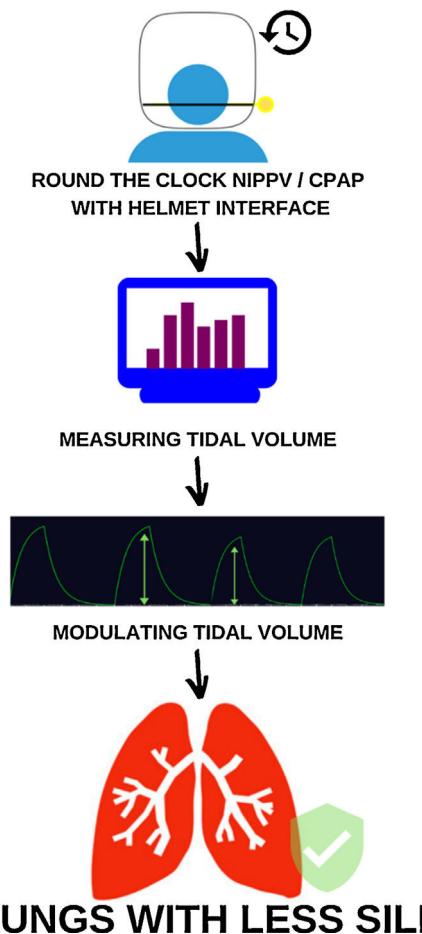

**Figure 1** Modulating tidal volume in NIPPV/CPAP spontaneous breathing patients can reduce SILI.

Mechanism of reducing SILI through measuring and modulating V<sub>t</sub> during round the clock cycles of mechanical ventilation with helmet interface.

CPAP: Continuous positive airway pressure; NIPPV: Noninvasive positive pressure ventilation; SILI: Self-induced lung injury.

NIV, at higher PEEP, compared to mask NIV, possibly resulting in a lower rate of endotracheal intubation. However, although interesting in term of comfort and in avoiding skin breakdown, the helmet has restrictions in measuring V<sub>t</sub> due to its mechanical properties.<sup>16</sup>

We recently tested the hypothesis<sup>17</sup> that TDV coupled with a single limb ILC, setting intentional leak location at the helmet expiratory port,<sup>18</sup> would provide patient's V<sub>t</sub> estimates. This configuration allows using the helmet even in

continuous positive airway pressure (CPAP) mode without additional rebreathing,<sup>18</sup> as in ICU ventilator in double limb configuration.<sup>19</sup> Results of the bench simulation in restrictive conditions (Table 1<sup>17</sup>) show that we could potentially use helmet NIV knowing  $V_t$ . Besides, differences in  $V_t$  between TDV and lung simulator remained stable across different tested leak flows.

This feasibility bench and human study demonstrated that estimating  $V_t$  during helmet NIV seems to be feasible and accurate in restrictive conditions. Although there are now questions about use of NIV in AHRF, the possibility of continuous noninvasive support for patients, knowing  $V_t$ , even in CPAP mode, could open new scenarios (Fig. 1), especially in "difficult-to-treat" hypoxicemic patients, such as in major burns<sup>20</sup> or in the immunocompromised.<sup>21</sup> Further clinical studies are required to verify this method.

## Funding

None.

## Authors' contribution

AC, MI, ML, CG conceived the content, wrote the manuscript and approved the last version.

## Declarations of interests

AC has a patent pending N° 102019000020532 related to the content of this manuscript; MI declare to have no competing interests; ML received fees for lectures and consultancies from Breas, Philips and Resmed not related to the resent work; CG received fees for lectures or consultancies from Philips, Resmed, Vivisol, Air Liquide not related to the present work, and has a patent pending N° 102019000020532 related to the content of this manuscript.

## References

- Gregoretti C, Pisani L, Cortegiani A, Ranieri VM. Noninvasive ventilation in critically ill patients. *Crit Care Clin.* 2015;31(July (3)):435–57.
- Cortegiani A, Russotto V, Antonelli M, Azoulay E, Carlucci A, Conti G, et al. Ten important articles on noninvasive ventilation in critically ill patients and insights for the future: a report of expert opinions. *BMC Anesthesiol.* 2017;17(September (1)):122.
- Ceriana P, Nava S, Vitacca M, Carlucci A, Panerini M, Schreiber A, et al. Noninvasive ventilation during weaning from prolonged mechanical ventilation. *Pulmonology.* 2019;25(6):328–33.
- Vaschetto R, Longhini F, Persona P, Ori C, Stefani G, Liu S, et al. Early extubation followed by immediate noninvasive ventilation vs. standard extubation in hypoxicemic patients: a randomized clinical trial. *Intensive Care Med.* 2019;45(January (1)):62–71.
- Bellani G, Laffey JG, Pham T, Madotto F, Fan E, Brochard L, et al. Noninvasive ventilation of patients with acute respiratory distress syndrome. Insights from the LUNG SAFE study. *Am J Respir Crit Care Med.* 2017;195(January (1)):67–77.
- Gregoretti C, Cortegiani A, Raineri SM, Giarratano A. Noninvasive ventilation in hypoxicemic patients: an ongoing soccer game or a lost one? *Turk J Anaesthesiol Reanim.* 2017;45(December (6)):329–31.
- Rochwerg B, Brochard L, Elliott MW, Hess D, Hill NS, Nava S, et al. Official ERS/ATS clinical practice guidelines: noninvasive ventilation for acute respiratory failure. *Eur Respir J.* 2017;50(Aug (2)):1602426.
- Brochard L, Slutsky A, Pesenti A. Mechanical ventilation to minimize progression of lung injury in acute respiratory failure. *Am J Respir Crit Care Med.* 2017;195(February (4)):438–42.
- Carteaux G, Millan-Guilarte T, De Prost N, Razazi K, Abid S, Thille AW, et al. Failure of noninvasive ventilation for de novo acute hypoxicemic respiratory failure: role of tidal volume. *Crit Care Med.* 2016;44(February (2)):282–90.
- Frat J-P, Ragot S, Coudroy R, Constantin J-M, Girault C, Prat G, et al. Predictors of intubation in patients with acute hypoxicemic respiratory failure treated with a noninvasive oxygenation strategy. *Crit Care Med.* 2018;46(February (2)):208–15.
- Carlucci A, Schreiber A, Mattei A, Malovini A, Bellinati J, Ceriana P, et al. The configuration of bi-level ventilator circuits may affect compensation for non-intentional leaks during volume-targeted ventilation. *Intensive Care Med.* 2013;39(January (1)):59–65.
- Lyazidi A, Thille AW, Carteaux G, Galia F, Brochard L, Richard J-CM. Bench test evaluation of volume delivered by modern ICU ventilators during volume-controlled ventilation. *Intensive Care Med.* 2010;36(December (12)):2074–80.
- Masselli GMP, Silvestri S, Sciuto SA, Cappa P. Circuit compliance compensation in lung protective ventilation. *Conf Proc IEEE Eng Med Biol Soc.* 2006;1:5603–6.
- Lujan M, Lalmolda C, Ergen B. Basic concepts for tidal volume and leakage estimation in non-invasive ventilation. *Turk Thorac J.* 2019;20(April (2)):140–6.
- Carteaux G, Lyazidi A, Cordoba-Izquierdo A, Vignaux L, Jolliet P, Thille AW, et al. Patient-ventilator asynchrony during noninvasive ventilation: a bench and clinical study. *Chest.* 2012;142(August (2)):367–76.
- Patel BK, Wolfe KS, Pohlman AS, Hall JB, Kress JP. Effect of noninvasive ventilation delivered by helmet vs face mask on the rate of endotracheal intubation in patients with acute respiratory distress syndrome: a randomized clinical trial. *JAMA.* 2016;315(June (22)):2435–41.
- Cortegiani A, Navalesi P, Accurso G, Sabella I, Misseri G, Ippolito M, et al. Tidal volume estimation during helmet noninvasive ventilation: an experimental feasibility study. *Sci Rep.* 2019;9(November (1)):17324.
- Racca F, Appendini L, Gregoretti C, Varese I, Berta G, Vittone F, et al. Helmet ventilation and carbon dioxide rebreathing: effects of adding a leak at the helmet ports. *Intensive Care Med.* 2008;34(August (8)):1461–8.
- Taccone P, Hess D, Caironi P, Bigatello LM. Continuous positive airway pressure delivered with a "helmet": effects on carbon dioxide rebreathing. *Crit Care Med.* 2004;32(October (10)):2090–6.
- Gregoretti C, Decaroli D, Piacevoli Q, Mistretta A, Barzaghi N, Luxardo N, et al. Analgo-sedation of patients with burns outside the operating room. *Drugs.* 2008;68(17):2427–43.
- Cortegiani A, Madotto F, Gregoretti C, Bellani G, Laffey JG, Pham T, et al. Immunocompromised patients with acute respiratory distress syndrome: secondary analysis of the LUNG SAFE database. *Crit Care.* 2018;22(June (1)):157.